


## Configuration Settings for Log Tag Thermometers

To configure your Log Tag thermometer:

1. Place your LogTag into the cradle to download temperatures or to set up a new LogTag for recording temperatures
2. Click on Log Tag in the upper menu bar of the Log Tag Analyzer program window and select Configure

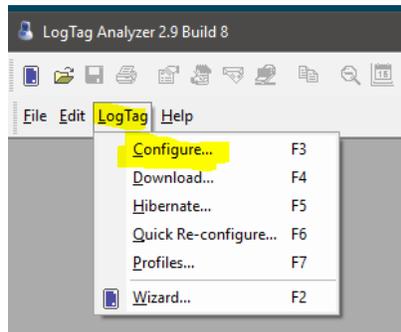

3. A Log Tag Configure window will open – make sure the settings are correct as shown below
  - Refrigerator Alarm Settings
    - Record a reading every 10 minutes
    - Trigger alarm when readings are above/equal to refrigerator setting of 46.5°F
      - After 3 Consecutive readings
    - Trigger alarm when readings are below/equal to refrigerator setting of 35.5°F
      - After 2 Consecutive readings

- Freezer Alarm Settings
  - Record a reading every 10 minutes
  - Trigger alarm when readings are above/equal to freezer setting of 5.5° F
    - After 3 Consecutive readings
  - Trigger alarm when readings are below/equal to freezer setting of -40° F
    - After 2 Consecutive readings

The screenshot shows the 'LogTag Configure' window with the following settings:


- User ID:** Freezer
- Action List:**
  - 1. Locate and identify LogTag(s) [checked]
  - 2. Configure LogTag(s) for next use [active]
  - 3. Prepare LogTag(s) for next use
- Start Method:** Push button start
- Battery Status:** LogTag battery: OK
- Logging Options:**
  - Enable pre-start logging
  - Record readings continuously, overwrite oldest when memory full
  - Record readings so that:
    - Readings recorded will span at least 110 days
    - Number of readings to record 15,905 (maximum is 15905)
- Recording Frequency:** Record a reading every 10 Minutes
- Delay:** Begin recording after a delay of 0 Minutes
- Alarm Settings:**
  - Trigger alarm when readings above/equal 5.5 °F
    - After 3 Consecutive violation readings (30 Minutes)
    - Audible alarm
  - Trigger alarm when readings below/equal -40 °F
    - After 2 Consecutive violation readings (20 Minutes)
    - Audible alarm
- Security:**
  - Configure requires a password
  - Download requires a password
- Buttons:** < Back, Next >, Close, Help, Advanced Options

## Advanced Options

Click on the Advanced Options button to view more setting options and enable the following options

- Check the box for the alarm to remain on after an alarm
- Temperature display unit: Fahrenheit
- Allow logging stop with Stop button
- Show total summary days collected

Click OK to save

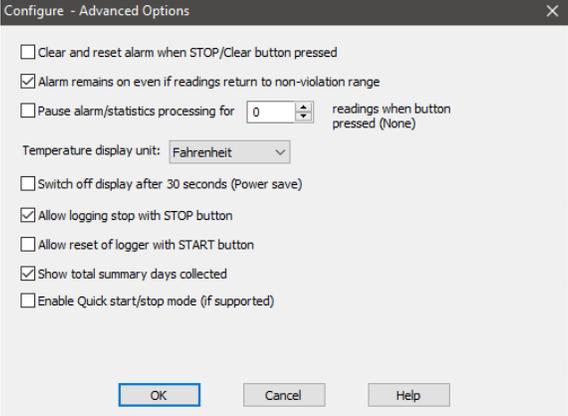

Configure - Advanced Options

- Clear and reset alarm when STOP/Clear button pressed
- Alarm remains on even if readings return to non-violation range
- Pause alarm/statistics processing for  readings when button pressed (None)
- Temperature display unit:
- Switch off display after 30 seconds (Power save)
- Allow logging stop with STOP button
- Allow reset of logger with START button
- Show total summary days collected
- Enable Quick start/stop mode (if supported)

OK Cancel Help